

Content available at: <https://www.ipinnovative.com/open-access-journals>

IP Indian Journal of Neurosciences

Journal homepage: <https://www.ijonline.org/>

Original Research Article

Beta initiated advanced closed loop DBS devices in achieving movement in Parkinson's

Siva Skandha Sanagala^{1*}, V Rama Raju^{1,2,3}¹CMR College of Engineering & Technology, Hyderabad, Telangana, India²Nizam's Institute of Medical Sciences, NIMS Hospital, Hyderabad, Telangana, India³CMR Institute of Medical Sciences, and CMR Hospital Kandlakoya, Hyderabad, Telangana, India

ARTICLE INFO

Article history:

Received 10-04-2024

Accepted 21-06-2024

Available online 27-06-2024

Keywords:

Adaptive deep brain stimulation (ACLDBS)
 Parkinson's disease (PD)
 Reaching movement
 Subthalamic nucleus
 β power
 Gamma power

ABSTRACT

Background: In Parkinson disease there is a normal physiological reduction of STN- β -band power, shorter smoothing period could have the advantage of being more sensitive to changes in β power, which could enhance motor performance. Objective: In this study, we addressed this question by evaluating effectiveness of STN- β -triggered ACL-DBS by a standard 400ms and a shorter 200ms smoothing-window during reaching movements.

Materials and Methods: Findings of Parkinson's with advanced idiopathic Parkinson's disease showed that reducing the smoothing-window for quantifying β did lead to shortened β -burst-durations by increasing number of β -bursts <200ms and more frequent switching "ON/OFF" of the stimulator but had no behavioral effects. Both ACL-DBS, COL-DBS improved motor performance to an equivalent extent compared to no DBS. Also, there were indemarkerdent effects of a decrease in β power and an increase in gamma power in predicting faster movement speed, while a decrease in β event-related-desynchronization (ERD) predicted quicker movement initiation. COL-DBS blocked both β and gamma (γ) more than ACL-DBS, whereas β ERD was reduced to a similar level during COL-DBS and ACL-DBS compared with no DBS, which together explained the achieved similar performance improvement in reaching movements during COL-DBS and ACL-DBS.

Results: Results suggesting STN- β -triggered ACL-DBS is effective in improving motor performance during reaching movements in people with Parkinson's disease, and that shortening of the smoothing window does not result in any additional behavioral benefit. When developing ACL-DBS systems for Parkinson's disease, it might not be necessary to track very fast β dynamics; combining β , gamma, and information from motor decoding might be more beneficial with additional bio-markers needed for optimal treatment of tremor.

Conclusion: This research is not just fundamentally designed to expand knowledge of basic mechanisms and principles of health and care problems. This is generally longer-term research with broad applicability and involves strategic, applied, developmental and implementation.

This is an Open Access (OA) journal, and articles are distributed under the terms of the [Creative Commons Attribution-NonCommercial-ShareAlike 4.0 License](https://creativecommons.org/licenses/by-nc-sa/4.0/), which allows others to remix, tweak, and build upon the work non-commercially, as long as appropriate credit is given and the new creations are licensed under the identical terms.

For reprints contact: reprint@ipinnovative.com

1. Introduction

In Parkinson's brain the electrophysiological patterns (signatures) alter due to numerous factors, such as age,

disease, environmental changes (phenotype) and genetic (change of DNA genes and genome) which is genotype. The subthalamic nucleus (STN) and globus pallidus (DP) are the two major elements to examine in Parkinson's disease (PD). So, researcher's aimed at these two neurons with deep brain stimulators and acquiring these neurons

* Corresponding author.

E-mail address: drvenkateshwararr@gmail.com (S. S. Sanagala).

signals with microelectrode recording machine. The DBS has been playing a pivotal role since last 2 decades and demonstrated a most successful therapeutic surgical procedure largely in patients with advanced idiopathic Parkinson's disease (PD).¹ The advanced adaptive closed loop deep brain stimulator (ACL-DBS) has been established to yield the progress of clinical diagnosis analogous to usual conventional (continuous) marker loop DBS (COL-DBS) with low-current delivered to brain plus less stimulus induced dyskinesias (related side-effects), postural instability, rigidity, akinesia (Bradykinesia) and tremor, loss of cognition (cognitive impairment CD), cognitive dementia (CD) plus reduced speech articulatory.^{2,3}

In PD, β activity is considered as a neural biomarker that correlates with the motor impairment, β is however not present in every patient. While PD is a chronic progressive disorder, the most important determinant of clinical progression is advancing age rather than disease duration. Preliminary findings from us show that calendar age is associated with a reduction in β power in the subthalamic nucleus (STN). The following can be suggested: the impacts of disease-process also age over electrophysiological activity, particularly on β activity, involve a biologic interaction.

Augmented synchronization of β -activity within STN steadily seen in people suffering through PD, also concurrent progressively through akinesia (i.e., Bradykinesia) plus stiffness/rigidity. Equally, progress in motoric-akinesia plus stiffness while medication ON and/or DBS ON is clearly linked with inhibition or suppression of β -power.⁴⁻⁹ Of late, compound findings have highlighted the significance of the temporal (progressive, of time) dynamics of STN- β fluctuations, in which the circumstance of prolonged and sustained β -bursts are absolutely associated with cardinal motoric loss.¹⁰⁻¹³ Collectively these results imply that the STN β activity is a marker (i.e., the bio marker) for Parkinsonian motoric signs which inspired and swayed the progress of β -triggered adaptive closed loop DBS (ACL-DBS) algorithms, objectively advancing the healing efficacy satisfactorily whilst reducing dyskinesias. The outcomes of numerous preliminary testing's of ACL-DBS through momentarily expressed stimulus electrodes,^{8,14-20} otherwise continually rooted or set in stimulus-devices especially DBS²¹ direct that β -triggered ACL-DBS, wherein the stimulus intensity (amplitude pulse-width) is attuned built on real-time multi-channel STN β -power approximation, is at best as real as predictable COL-DBS in plummeting motoric-signs inactive and stationary as assessed subjectively falling under the score of 6.

Yet, numerous question-marks persist unreciprocated. Primarily, does β -generated ACL-DBS cause damaging functioning for attaining movements assessed through COL-DBS in Parkinson's? There is a STN- β activity reduction

biologically and functionally (i.e., physiologically) in controlled movements, which could see in individuals with Parkinson's disease²²⁻²⁴ which can also lead to reduction or cessation of stimuli whilst movement in the setup of β -generated ACL-DBS which may conciliate motor functioning associated through COL-DBS if at all more β conquest (clampdown) in movement is obliging and very much supportive to the benefits of therapy maximally whilst subjects challenge movements, i.e., once they want it highly and possibly and perchance.²⁵ Secondly, is compelling ACL-DBS highly reactive to β -fluctuations by momentarily window-smoothing technique for quantifying the β power result in improving the motor execution well? In order to establish and estimate the β , the window-smoothing is an important parameter which desires to be measured whilst evolving the advanced ACL-DBS device, because diverse 'windows-smoothing' change the dynamics of influences amid stimuli plus generated oscillatory-fluctuations. Present research articles β -activated ACL-DBS have projected β power in simultaneous devices (the amount of processing that can be accomplished during interval of time, in the given interval of time) by applying the 'moving-window- averaging (MWA)' of 400-ms interval or retentive, meant for β acquisition bursts for elongated intervals largely.^{10,14-16}

Earlier researchers²⁶ through the particular trial investigations of local field potentials (LFPs) gathered as of corpus striatum (striate-body) plus motoric and pre motor-cortex in primates exhibited that short-lived(transitory) ruptures-of-oscillatory fluctuations with an interval of 50ms–150ms are accountable for pragmatically all the β frequency band-activity, and which determined modulation's within the experimentally mean-averaged β stimulus-amplitudes mainly replicate reproduce the intonations (variations) of the ruptures or eruptions (burst)-densities which is consistent with findings of normal controls demonstrating that higher-amplitudes β -events as of somato sensory plus anterior/frontal motor-cortex stereo typically persisted <150ms also had a characteristic stereo typical non sinusoid's-phase.²⁷ Hence, we hypothesized that there can be spare aids of the advanced ACL-DBS algorithmic-procedure able to pruning STN- β actions and events in to even quicker torrents, as seen in controls sensori motor-cortex cortical basal ganglia (BG) network^{26,27} by the application of rapider window-smoothing algorithmic-technique duration (e.g. 200ms). To respond for all these issues, we built a new procedure merging a signaled achieving errand plus the brain machine interface (MBI) letting concurrent estimation parallelly for the STN- β as well as regulation of stimulus-amplitude (Figure 1) and guessed the motor execution in thirteen Parkinson's and in four changed stimulus-constraints OFF DBS, COL-DBS, ACL-DBS -400 (ACL-DBS with β stimulus-amplitude smoothed over 400ms), ACL-DBS -200 (ACL-DBS through

the β -power smoothed completed in 200 milliseconds).

2. Materials and Methods

2.1. Normal controls

Thirteen subjects with advanced idiopathic Parkinson's disease male female ratio 7:6 partaken to the experimental-investigation later being employed at our tertiary care hospital in Hyderabad, India (Table 1, clinical demographic). They undertook subthalamic nucleus deep brain stimulations bilaterally. Electrodes are summarized in Table 1 were provisionally conveyed preceding to the successive micro neurosurgery to link them to a neuro stimulator. Electrode implanted point of contacts were inveterated deeply-rooted through the blend of pre- op MR imaging and post op CAT scanning's, that were further inveterated via restructuring the microelectrode paths plus point of varied interactions by applying various Mat Lab toolboxes (R2022A, ver..8. with Simulink).^{28–39} Figure 1D, depicts largely checked sensors (microelectrode's) bundled in a satisfying point that has been advocated to give complete beat and ideal motor perfection to Parkinson's through the stimulations.^{40–49} There one single microelectrode hap markers designate at the edge of sub thalamic nucleus (Figure 1,P1L), thus we employed "volume-of tissue-activated" (VTA) investigation via stimulus-parameters like intensity amplitude, pulse-width, and frequency as employed for the acquisition of data through this sensor (i.e., microelectrode).^{50–60}

Which conforms those stimulations given to the microelectrodes which led to the V T A that coincided the nucleus-STN and the thoughtful bit for inclusive motoric-progression. Institute ethical approval obtained, and Helsinki principle followed, plus every subject is given written permission. The mean age at the onset was 62.15 ± 1.58 years (mean \pm SEM), duration-of-disease is 10 ± 1.21 years, response to the medicine (mean-scoring of MDS-UPDRS stage-III 37.04 ± 2.95 (MED-OFF), 12.42 ± 1.67 (MED-ON), correspondingly. The medicine was off during the experiment. Fill

2.2. Investigational procedure

The procedure involved two stages, an indication (cued) 'reaching-task' through a marker (automated), and a 20second finger-tapping. Each test (Figure 1A) of the 'reaching-task' pioneered through the demonstration of a grey-filled-sphere (at posterior of computer-system-monitor) signaling that the subject must carry the marker to initial point when que is set. When, the instant, the biomarker is in the initial point, the orbit turns emerald-green to show that the biomarker is uncovered. Following the irregular and mutable interval of (i.e., pause) of 1 to 2seconds, a saffron-bursting orbit, which is termed "go-cue" occurred, over the 3prospective aimed locations,

namely, "top - left", "top - middle" and/or "top - right" of the computer display screen, i.e., monitor. After this "go-cue-signal", the subject is directed to accomplish the aimed-object, i.e., target-object, return to starting point as swiftly as feasible. The Figure 1B, demonstrates the entire experiment comprising the 8-blocksof 15-testsby the entomb (or intomb) test intervals of 4s to 5seconds randomised. and 2-blocks are there in every 4-tested trials stimulus states (DBS-OFF: COL-DBS, ACL-DBS-200, ACL-DBS-400).^{51–61} Therefore, after

Achieving the task of movement, and at the end of each block, the subject was directed to do finger-tapping activities for few seconds, i.e., 20s by utilizing their index-fingers on their browse through, flip-through as wide and fast as possible. Following the changes at every situation, the average-mean interval-of 67.67 ± 9.20 seconds (mean \pm SEM) comprised prior to beginning the fresh-block for cleaning out the likely stimulus-effect as of previous block. In-full, signal acquisitions through every subject endured till 3hours for left and right hemispheres/or 120 minutes for unilateral (hemisphere). Order-of experiment investigational-blocks are pseudo-randomized plus counter-balanced across subjects. For attaining this, and for every subject, the any 4 blocks encompassed the 4 stimulus constraints in the order of randomization, plus/ as well as 4 constraints are recurrent within the inverse direction within the dualistic 4 blocks (Figure 1B).^{61–65}

2.3. Electrical-stimulations

The electrical-stimulations were given one side of the brain, i.e., unilateral, i.e., to the brins hemi sphere contra lateral to hands-fingers accomplishing the work. A substantially and technically specifications configurable custom-built neuro stimulator and certified was employed to deliver continuous current stimulations within the monopolar mode. One-of two connections in center was applied as a stimulus connection, as well as the microelectrode spot assigned/screwed to the back-of subject was employed for reference-point-of view (Figure 1C).

2.4. Deciding and choosing stimulus-contacts, stimulus-intensity (voltage)/amplitude, β -band freq. for response

The β -band frequencies are used as feed-back-signals. Particularly, we delivered constant DBS to the centrally contacting and in the beginning at 0.5mA. Then we gradually enhanced stimulus-amplitudes in 0.5mA and 2-5voltage, pulse-width-60Hz, additions, till medical use was perceived with no dyskinesias for instance, paresthesia, and/or till 3.5mA was accomplished as the greatest amplitude-energy. If there is no visible medical result was examined, we echoed this process for next central-contact stage. By the time stimulus-contact and amplitude/stimulus-

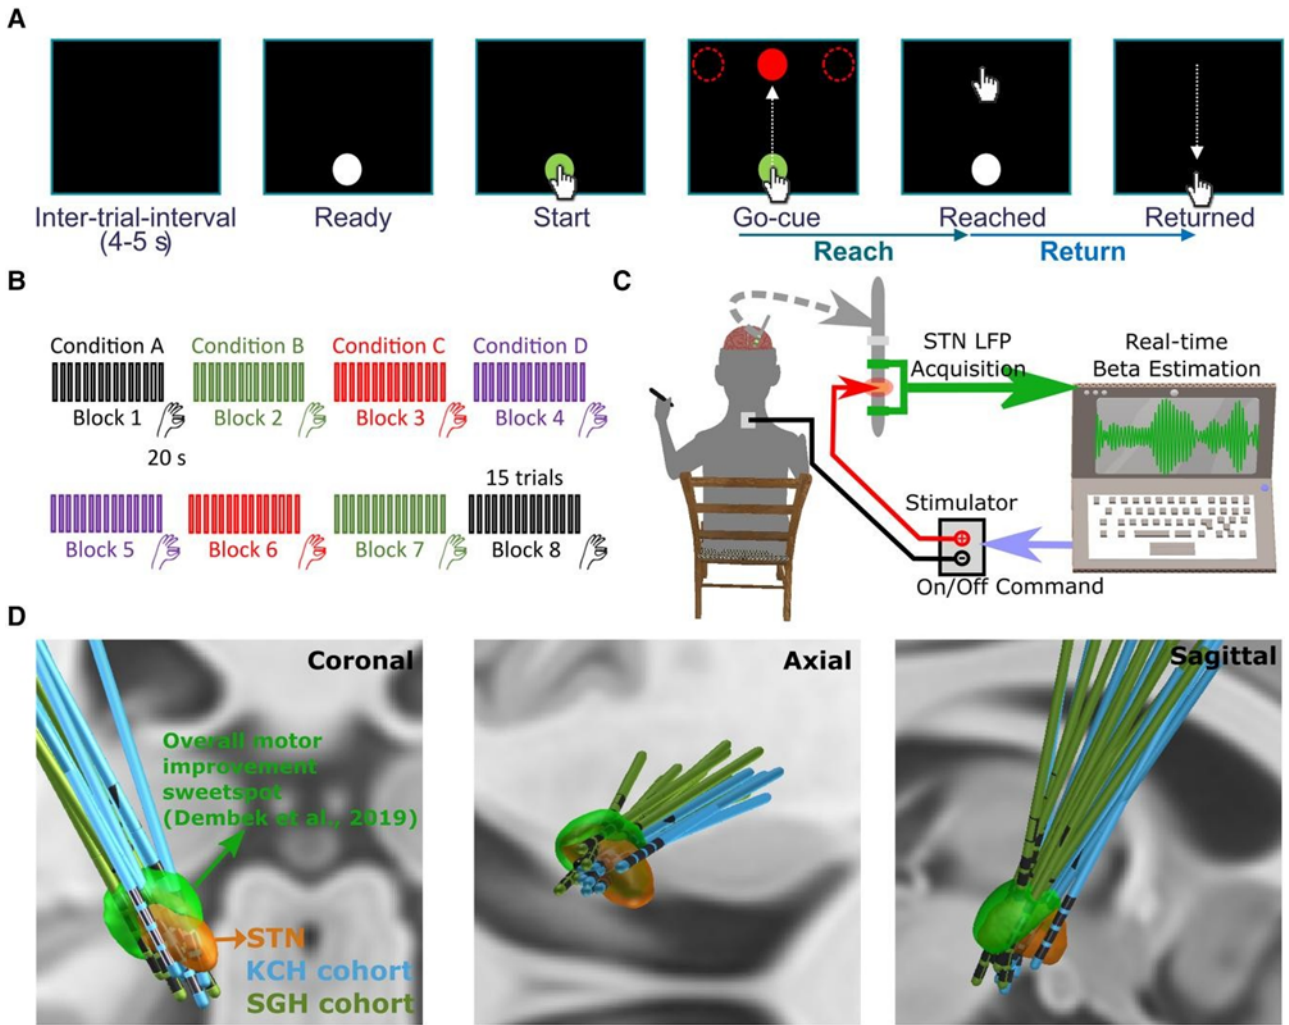


Figure 1: Experimental protocol. (A) Duration of single-test of achieving errand executed over the tangible display-screen using the markercil. In every-test, Parkinson is directed to spot at flinch (jolt) switch to start the test and to access to the red objective whilst the drive-cue is flashed plus return to jolt knob whilst the object flees, as faster as likely. (B) Duration for entire investigational (experiment) phase implies 8 deal with neutral (reasonable) wedges in 4 distinct stimulus settings, and 2wedges in every constraint. Every wedge consists of fifteen tests of range-reappearance activities after 20sec of digit-patter actions. (C) Representation of ACL-DBS device with bi-polar size-of STN-DBS LFPs, simultaneous estimate of β -power plus single electrode (unipolar, i.e., mono polar) stimuli supplied to one of the central-contacts, whilst Parkinson is easily sit in the chair, accomplish the given tasks. (D) 3dimensional restoration in left, middle plus right interpretations for all the analyzed microelectrodes.^{28,29} The sensors on left-hemi sphere were reflected to the right hemi sphere. Findings showed that all the verified sensors are grouped in a thoughtful bit which recommended to offer total ideal motoric enhancement for Parkinson’s through the deep brain stimulators (depicted in greenish color).³⁰

intensity were chosen, a period-of 2 minutes of stand gatherings (signal acquisitions through the MER) was accomplished. Local field potentials and beta oscillatory fluctuations are gathered/acquired (recorded with MER) as of 2connections adjacent the chosen stimulus contact within differential bipolar mode.^{66–69}

The stimulus parameters demonstrated in the Table1 were kept chronic for various stimulus constraints for all hemi spheres.

2.5. Clinico-statistical inferences

A clinic-statistical techniques for the analysis purposes were organized through the custom written scripts within the MatLabR2021-b.

For those system of measurements measured and determined over the per-constraint-basis which includes stimulus swapping-rate, mean-average % of-time during the DBS was ON, average-burst-duration as well as ‘burst-rate’, matching student t-tests were conducted to assess the outcome of the stimulus-constraint. Bell-shaped-

Table 1:

Case-event	Micro electrodes	Stimulus contact (L/R)	Investigation DBS			ONDBS	
			StimAmp (L/R, mA)	Bipolarfeedback channel(L/R)	Online-filter range (L/R Hz)	Stimulus Contact (L/R)	StimAmp (L/R)
1	Medtronic1	L-3a	3	L-24	19–25	L-2	3.3 V
2	Medtronic1	L-3 /R-2c	3.5/1.5	L-24/R-13	14–20/15–21	L-1/R-2	2.9/2.7mA
3	Boston1	L2c/R3c	3/2	L-13/R-24	15–21/14–20	-L2-L-3/R-2-R3	4.0/3.5mA
4	Boston2	L-3c	1	L-24	16–22	L-2-L3	4.2mA
5	Abbot	R-3a,	1.5	R-24	17–23	R-2	3.2mA
6	Medtronic2	R-2a	1.5	R-13	19–25	R-1	2.6mA
7	Boston3	L-2c/R-2c	2.5/2.5	L-13/R-13	16–22/22–28	L-2-L4/R2	2.8/2.3mA
8	Medtronic2	R-2c	3	R-13	15–21	R-2	3.6mA
9	Medtronic2	L-3a	1.5	L-24	14–20	-L4	2.5mA
10	Medtronic2	L-2c/R-2c	1/3	L-13/R-13	22–28/22–28	L-2/R2	2.4/3.5mA
11	Medtronic2	L-3a/R-2c	3.5/3.5	L-24/R-13	18–24/17–23	L-2/R2	1.9/1.7mA
12	Medtronic2	L-2c/R-2c	3/3	L-13/R-13	12–18/21–27	L-2/R2	1.0/1.0mA
13	Boston1	L-2c/R-2c	2/2	L-13/R-13	18–24/20–26	L-2-L3/R-2-R3	4.5/1.7mA
Mean-average	–	–	2.38	–	17.3–23.3	–	2.77
SEM	–	–	0.18	–	0.66	–	0.22

normal distribution guess was established by applying the “Anderson–Darling” testing’s. Numerous assessments for the differences were employed to numerous measurements were adjusted by applying the Bonferroni adjustment. For Every contrast the number-of-case-events, the student t-values as well as pre-modified. The P-values were reported<0.05 statistically significant.

3. Results

Results showed that reducing the smoothing window for quantifying β did lead to shortened β -burst durations by increasing the number of β bursts shorter than 200ms and more frequent switching “ON/OFF” of the stimulator but had no behavioral effects. Both ACL-DBS and COL-DBS improved motor performance to an equivalent extent compared to no “ON-DBS”. Secondary analysis revealed that there were indemarkerdent effects of a decrease in β power and an increase in gamma power in predicting faster movement speed, while a decrease in β event-related-de synchronization (ERD) predicted quicker movement initiation. COL-DBS blocked both β and gamma (γ) more than ACL-DBS, whereas β ERD was reduced to a similar level during COL-DBS and ACL-DBS compared with no DBS, which together explained the achieved similar performance improvement in reaching movements during COL-DBS and ACL-DBS. In addition, ACL-DBS significantly improved tremor compared with no DBS but was not as effective as COL-DBS. These results suggest that STN β - triggered ACL-DBS is effective in improving motor performance during reaching movements in people with Parkinson’s disease, and that shortening of

the smoothing window does not result in any additional behavioral benefit. When developing ACL-DBS systems for Parkinson’s disease, it might not be necessary to track very fast β dynamics; combining β , gamma, and information from motor decoding might be more beneficial with additional bio- markers needed for optimal treatment of tremor. This research is not just fundamentally designed to expand knowledge of basic mechanisms and principles of health and care problems. This is generally longer-term research with broad applicability and involves strategic, applied, developmental and implementation.

4. Conclusions

This study estimated the efficacy of the sub thalamic nucleus beta β -activated advanced adaptive closed loop deep brain stimulators (ACL-DBS) throughout the achieving mission concerning u p p e r-limb m o v e m e n t s within the 13subjects with advanced idiopathic Parkinson disease shaking palsy. We demonstrated that β -activated ACL-DBS devices were did not compromised the motoric execution of reaching (with the help of cue,i.e. cued) movements in rappsorts of response time as well as movement speed equated through the conventional open loop(COL-DBS) device. The two devices are substantially enhanced motoric-execution through the analogous amounts judged with no stimulations. Furthermore, we explained that by applying the quicker window-smoothing technique to assess the beta (β) oscillations did make ACL-DBS further approachable and reactive. It reduced β -bursts interval-periods by improving the numerous β -bursts concise than 200milliseconds, yet this didn’t give one

further advantage within the motor execution. Also we demonstrated that the two STN and β -reductions as well as gamma-energy-power strengthen throughout drive assisted in expecting the drive pace and speediness', signifying that compounding the β , γ as well as drive position may consult additional advantage in advanced adaptive ACL-DBS devices. Additionally, β -activated ACL-DBS device was not that much as applicable as that of the COL-DBS device in defeating the Parkinsonian rest/tremor or, advocating that supplementary responsive-feedback-signals can be obliged for shaking palsy and for dominant dominant tremors of the individuals-patients, i.e., Parkinson disease patients. The results in this study have noteworthy effects for extended enhancement of the ACL-DBS devices algorithmic-techniques to enhance the cure and to comprehend better Parkinson's disease.

5. Source of Funding

None.

6. Conflict of Interest

None.

References

- Deuschl G, Schade-Brittinger C, Krack P, Volkmann J, Schäfer H, Bötzel K, et al. A randomized trial of deep-brain stimulation for Parkinson's disease. *N Engl J Med*. 2006;355(9):896–908.
- Zangaglia R, Pacchetti C, Pasotti C, Mancini F, Servello D, Sinforiani E, et al. Deep brain stimulation and cognitive functions in Parkinson's disease: a three-year controlled study. *Mov Disord*. 2009;24(11):1621–8.
- Castrioto A, Lozano AM, Poon YY, Lang AE, Fallis M, Moro E, et al. Ten-year outcome of subthalamic stimulation in Parkinson disease: a blinded evaluation. *Arch Neurol*. 2011;68(12):1550–6.
- Kühn AA, Kupsch A, Schneider GH, Brown P. Reduction in subthalamic 8-35 Hz oscillatory activity correlates with clinical improvement in Parkinson's disease. *Eur J Neurosci*. 2006;23(7):1956–60.
- Kühn AA, Tsui A, Aziz T, Ray N, Brücke C, Kupsch A, et al. Pathological synchronisation in the subthalamic nucleus of patients with Parkinson's disease relates to both bradykinesia and rigidity. *Exp Neurol*. 2009;215(2):380–7.
- Neumann WJ, Degen K, Degen K, Brücke C, Huebl J, Brown P, et al. Subthalamic synchronized oscillatory activity correlates with motor impairment in patients with Parkinson's disease. *Mov Disord*. 2016;31(11):1748–51.
- Oswal A, Beudel M, Zrinzo L, Limousin P, Hariz M, Foltynie T, et al. Deep brain stimulation modulates synchrony within spatially and spectrally distinct resting state networks in Parkinson's disease. *Brain*. 2016;139(Pt 5):1482–96.
- Little S, Brown P. Debugging adaptive deep brain stimulation for Parkinson's disease. *Mov Disord*. 2020;35(4):555–61.
- Kehnemouyi YM, Wilkins KB, Anidi CM, Anderson RW, Afzal MF, Bronte-Stewart HM, et al. Modulation of β bursts in subthalamic sensorimotor circuits predicts improvement in bradykinesia. *Brain*. 2021;144(2):473–86.
- Tinkhauser G, Pogosyan A, Little S, Beudel M, Herz DM, Tan H, et al. The modulatory effect of adaptive deep brain stimulation on β bursts in Parkinson's disease. *Brain*. 2017;140(4):1053–67.
- Tinkhauser G, Pogosyan A, Tan H, Herz DM, Kühn AA, Brown P, et al. B-Burst dynamics in Parkinson's disease OFF and ON dopaminergic medication. *Brain*. 2017;140(11):2968–81.
- Tinkhauser G. The cumulative effect of transient synchrony states on motor performance in Parkinson's disease. *J Neurosci*. 2020;40:1571–1580.
- Torreclillos F. Modulation of β bursts in the subthalamic nucleus predicts motor performance. *J Neurosci*. 2018;38:8905–8917.
- Little S. Adaptive deep brain stimulation in advanced Parkinson disease. *Ann Neurol*. 2013;74:449–457.
- Little S, Beudel M, Zrinzo L, Foltynie T, Limousin P, Hariz M, et al. Bilateral adaptive deep brain stimulation is effective in Parkinson's disease. *J Neurol Neurosurg Psychiatry*. 2016;87(7):717–21.
- Herz DM, Little S, Pedrosa DJ, Tinkhauser G, Cheeran B, Foltynie T, et al. Mechanisms Underlying Decision-Making as Revealed by Deep-Brain Stimulation in Patients with Parkinson's Disease. *Curr Biol*. 2018;28(8):1169–78.
- Iturrate I, Martin S, Chavarriaga R, Orset B, Leeb R, Sobolewski A, et al. Beta-driven closed-loop deep brain stimulation can compromise human motor behavior in Parkinson's Disease. *bioRxiv*. 2019;doi:10.1101/696385.
- Piña-Fuentes D, van Dijk J, van Zijl J, Moes HR, Laar T, Oterdoom DLM, et al. Acute effects of adaptive Deep Brain Stimulation in Parkinson's disease. *Brain Stimul*. 2020;13(6):1507–16.
- Arlotti M. Eight-hours adaptive deep brain stimulation in patients with Parkinson disease. *Neurology*. 2018;90:971–976.
- Bocci T, Prenassi M, Arlotti M, Cogiamanian FM, Borellini L, Moro E, et al. Eight-hours conventional versus adaptive deep brain stimulation of the subthalamic nucleus in Parkinson's disease. *NPJ Parkinsons Dis*. 2021;7:88. doi:10.1038/s41531-021-00229-z.
- Gilron RE, Little S, Perrone R, Wilt R, Hemptinne C, Yaroshinsky MS, et al. Long-term wireless streaming of neural recordings for circuit discovery and adaptive stimulation in individuals with Parkinson's disease. *Nat Biotechnol*. 2021;39(9):1078–85.
- Kühn AA, Williams D, Kupsch A, Limousin P, Hariz M, Schneider GH, et al. Event-related β desynchronization in human subthalamic nucleus correlates with motor performance. *Brain*. 2004;127(Pt 4):735–46.
- Jenkinson N, Brown P. New insights into the relationship between dopamine, β oscillations and motor function. *Trends Neurosci*. 2011;34(12):611–8.
- Oswal A, Litvak V, Brücke C, Huebl J, Schneider GH, Kühn AA, et al. Cognitive factors modulate activity within the human subthalamic nucleus during voluntary movement in Parkinson's disease. *J Neurosci*. 2013;33(40):15815–26.
- Darbin O, Hatanaka N, Takara S. Subthalamic nucleus deep brain stimulation driven by primary motor cortex γ 2 activity in parkinsonian monkeys. *Sci Rep*. 2022;12:6493. doi:10.1038/s41598-022-10130-1.
- Feingold J, Gibson DJ, DePasquale B, Graybiel AM. Bursts of β oscillation differentiate postperformance activity in the striatum and motor cortex of monkeys performing movement tasks. *Proc Natl Acad Sci USA*. 2015;112(44):13687–92.
- Sherman MA, Lee S, Law R, Haegens S, Thorn CA, Hämläinen MS, et al. Neural mechanisms of transient neocortical β rhythms: converging evidence from humans, computational modeling, monkeys, and mice. *Proc Natl Acad Sci USA*. 2016;113(33):4885–94.
- Avants BB, Epstein CL, Grossman M, Gee JC. Symmetric diffeomorphic image registration with cross-correlation: evaluating automated labeling of elderly and neurodegenerative brain. *Med Image Anal*. 2008;12(1):26–41.
- Horn A, Li N, Dembek TA, Kappel A, Boulay C, Ewert S, et al. Lead-DBS v2: towards a comprehensive pipeline for deep brain stimulation imaging. *Neuroimage*. 2019;184:293–316. doi:10.1016/j.neuroimage.2018.08.068.
- Dembek TA. Probabilistic sweet spots predict motor outcome for deep brain stimulation in Parkinson disease. *Ann Neurol*. 2019;86:527–538.
- Ansó J, Benjaber M, Parks B, Parker S, Oehr CR, Petrucci M, et al. Concurrent stimulation and sensing in bi-directional brain interfaces: a multi-site translational experience. *J Neural Eng*. 2022;19(2). doi:10.1088/1741-2552/ac59a3.

32. Meidahl AC. Adaptive deep brain stimulation for movement disorders: the long road to clinical therapy. *Mov Disord.* 2017;32(6):810–9.
33. Stamatakis J, Ambroise J, Crémers J, Sharei H, Delvaux V, Macq B, et al. Finger tapping clinical score prediction in Parkinson's disease using low-cost accelerometers. *Comput Intell Neurosci.* 2013;p. 717853. doi:10.1155/2013/717853.
34. Van Dennoort J, Verhagen R, van Dijk K, Veltink PH, Vos M, de Bie R, et al. Quantification of hand motor symptoms in Parkinson's disease: a proof-of-principle study using inertial and force sensors. *Ann Biomed Eng.* 2017;45(10):2423–36.
35. He S, Mostofi A, Syed E, Torrecillos F, Tinkhauser G, Fischer P, et al. Subthalamic β -targeted neuro-feedback speeds up movement initiation but increases tremor in parkinsonian patients. *Elife.* 2020;9:e60979. doi:10.7554/eLife.60979.
36. Lo S, Andrews S. To transform or not to transform: using generalized linear mixed models to analyse reaction time data. *Front Psychol.* 2015;6:1171. doi:10.3389/fpsyg.2015.01171.
37. Maris E, Oostenveld R. Nonparametric statistical testing of EEG- and MEG-data. *J Neurosci Methods.* 2007;164(1):177–90.
38. Wiest C, Tinkhauser G, Pogosyan A, Bange M, Muthuraman M, Groppa S, et al. Local field potential activity dynamics in response to deep brain stimulation of the subthalamic nucleus in Parkinson's disease. *Neurobiol Dis.* 2020;143:105019. doi:10.1016/j.nbd.2020.105019.
39. Lofredi R, Okudzhava L, Irmen F, Brücke C, Huebl J, Krauss JK, et al. Subthalamic β bursts correlate with dopamine-demarkerdent motor symptoms in 106 Parkinson's patients. *NPJ Parkinsons Dis.* 2023;9(1):2. doi:10.1038/s41531-022-00443-3.
40. Deffains M, Iskhakova L, Katabi S, Israel Z, Bergman H, et al. Longer β oscillatory episodes reliably identify pathological subthalamic activity in parkinsonism. *Mov Disord.* 2018;33(10):1609–18.
41. Echeverria-Altuna I, Quinn AJ, Zokaei N, Woolrich MW, Nobre AC, Ede F, et al. Transient beta activity and cortico-muscular connectivity during sustained motor behaviour. *Prog Neurobiol.* 2022;214:102281. doi:10.1016/j.pneurobio.2022.102281.
42. Pfurtscheller G, Stancák A, Neuper C. Post-movement β synchronization: a correlate of an idling motor area? *Electroencephalogr Clin Neurophysiol.* 1996;98(4):281–93.
43. Chen R, Yaseen Z, Cohen LG, Hallett M. Time course of corticospinal excitability in reaction time and self-paced movements. *Ann Neurol.* 1998;44(3):317–25.
44. Wessel JR, Ghahremani A, Udupa K, Saha U, Kalia S, Hodaie M, et al. Stop-related subthalamic beta activity indexes global motor suppression in Parkinson's disease. *Mov Disord.* 2016;31(12):1846–53.
45. Ray NJ, Brittain JS, Holland P, Joundi RA, Stein JF, Aziz TZ, et al. The role of the subthalamic nucleus in response inhibition: evidence from local field potential recordings in the human subthalamic nucleus. *Neuroimage.* 2012;60(1):271–8.
46. Tan H, Pogosyan A, Anzak A, Ashkan K, Bogdanovic M, Green AL, et al. Complementary roles of different oscillatory activities in the subthalamic nucleus in coding motor effort in parkinsonism. *Exp Neuro.* 2013;248:187–95. doi:10.1016/j.expneurol.2013.06.010.
47. Anzak A, Tan H, Pogosyan A, Foltynie T, Limousin P, Zrinzo L, et al. Subthalamic nucleus activity optimizes maximal effort motor responses in Parkinson's disease. *Brain.* 2012;135(Pt 9):2766–78.
48. Lofredi R, Neumann WJ, Bock A, Horn A, Huebl J, Siegert S, et al. Dopamine-demarkerdent scaling of subthalamic gamma bursts with movement velocity in patients with Parkinson's disease. *Elife.* 2018;7:31895. doi:10.7554/eLife.31895.
49. Brücke C, Huebl J, Schönecker T, Neumann WJ, Yarrow K, Kupsch A, et al. Scaling of movement is related to pallidal γ oscillations in patients with dystonia. *J Neurosci.* 2012;32(3):1008–19.
50. Kühn AA, Kempf F, Brücke C, Doyle LG, Torres IM, Pogosyan A, et al. High-frequency stimulation of the subthalamic nucleus suppresses oscillatory beta activity in patients with Parkinson's disease in parallel with improvement in motor performance. *J Neurosci.* 2008;28(24):6165–73.
51. Eusebio A, Thevathasan W, Gaynor D, Pogosyan A, By E, Foltynie T, et al. Deep brain stimulation can suppress pathological synchronization in parkinsonian patients. *J Neurol Neurosurg Psychiatry.* 2011;82(5):569–73.
52. Little S, Brown P. What brain signals are suitable for feedback control of deep brain stimulation in Parkinson's disease? *Ann N Y Acad Sci.* 2012;1265(1):9–24.
53. Velisar A, Syrkin-Nikolau J, Blumenfeld Z, Trager MH, Afzal M, Prabhakar V, et al. Dual threshold neural closed loop deep brain stimulation in Parkinson disease patients. *Brain Stimul.* 2019;12(4):868–76.
54. Qasim SE, Hemptinne C, Swann N, Miocinovic S, Ostrem JL, Starr P, et al. Electroencephalography reveals β desynchronization in the basal ganglia-cortical loop during rest tremor in Parkinson's disease. *Neurobiol Dis.* 2016;86:177–86. doi:10.1016/j.nbd.2015.11.023.
55. Wang SY, Aziz TZ, Stein JF, Liu X. Time-frequency analysis of transient neuromuscular events: dynamic changes in activity of the subthalamic nucleus and forearm muscles related to the intermittent resting tremor. *J Neurosci Methods.* 2005;145(1-2):151–8.
56. Hirschmann J, Hartmann CJ, Butz M, Hoogenboom N, Ozkurt TE, Elben S, et al. A direct relationship between oscillatory subthalamic nucleus-cortex coupling and rest tremor in Parkinson's disease. *Brain.* 2013;136(Pt 12):3659–70.
57. Debarros J, Gaignon L, He S, Pogosyan A, Benjaber M, Denison T, et al. Artefact-free recording of local field potentials with simultaneous stimulation for closed-loop deep-brain stimulation. *Annu Int Conf IEEE Eng Med Biol Soc.* 2020;p. 3367–70. doi:10.1109/EMBC44109.2020.9176665.
58. He S, Baig F, Mostofi A, Pogosyan A, Debarros J, Green AL, et al. Closed-loop deep brain stimulation for essential tremor based on thalamic local field potentials. *Mov Disord.* 2021;36(4):863–73.
59. Tan H, Debarros J, He S, Pogosyan A, Aziz TZ, Huang Y, et al. Decoding voluntary movements and postural tremor based on thalamic LFPs as a basis for closed-loop stimulation for essential tremor. *Brain Stimul.* 2019;12(4):858–67.
60. Opri E. Chronic embedded cortico-thalamic closed-loop deep brain stimulation for the treatment of essential tremor. *Sci Transl Med.* 2020;12(572):7680. doi:10.1126/scitranslmed.aay7680.
61. Merk T, Peterson V, Lipski WJ, Blankertz B, Turner RS, Li N, et al. Electroencephalography is superior to subthalamic local field potentials for movement decoding in Parkinson's disease. *Elife.* 2022;11:e75126. doi:10.7554/eLife.75126.
62. Swann NC, Hemptinne C, Miocinovic S, Qasim S, Wang SS, Ziman N, et al. Gamma oscillations in the hyperkinetic state detected with chronic human brain recordings in Parkinson's disease. *J Neurosci.* 2016;36(24):6445–58.
63. Gilron RE, Little S, Wilt R, Perrone R, Anso J, Starr P, et al. Sleep-aware adaptive deep brain stimulation control: chronic use at home with dual indemarkerdent linear discriminate detectors. *Front Neurosci.* 2021;15:732499. doi:10.3389/fnins.2021.732499.
64. Vaou OE, Spidi MD, Raïke R, Moises A, Stanslaski S, Case M, et al. Symptom optimization through sensing local field potentials: balancing β and gamma in Parkinson's disease. *Deep Brain Stimulation.* 2023;1:5–14. doi:10.1016/j.jdbs.2023.01.001.
65. Blumenfeld Z, Koop M, Prieto TE, Shreve LA, Velisar A, Quinn E, et al. Sixty-hertz stimulation improves bradykinesia and amplifies subthalamic low-frequency oscillations. *Mov Disord.* 2017;32(1):80–8.
66. Moreau C, Pennel-Ployart O, Pinto S, Plachez A, Annic A, Viallet F, et al. Modulation of dysarthropneumophonia by low-frequency STN DBS in advanced Parkinson's disease. *Mov Disord.* 2011;26(4):659–63.
67. Xie T, Vigil J, MacCracken E, Gasparaitis A, Young J, Kang W, et al. Low-frequency stimulation of STN-DBS reduces aspiration and freezing of gait in patients with PD. *Neurology.* 2015;84(4):415–20.
68. Xie T, Padmanaban M, Bertacchi B, Kang W, MacCracken E, Dachman A, et al. Long-term effect of low frequency stimulation of STN on dysphagia, freezing of gait and other motor symptoms in PD. *J Neurol Neurosurg Psychiatry.* 2018;89(9):989–94.

69. Wiest C, Torrecillos F, Tinkhauser G, Pogosyan A, Morgante F, Pereira EA, et al. Finely-tuned gamma oscillations: spectral characteristics and links to dyskinesia. *Exp Neurol*. 2022;351:113999. doi:10.1016/j.expneurol.2022.113999.

V Rama Raju, Professor

Author biography

Siva Skandha Sanagala, Professor

Cite this article: Sanagala SS, Raju VR. Beta initiated advanced closed loop D B S devices in achieving movement in Parkinson's. *IP Indian J Neurosci* 2024;10(2):93-100.